

Customer Care Representative:

Line No.

Order No.

**Fits: AGILITY Minimum Contour 20" Width x 16" Height x 3" Depth**

## How to Use the Custom AGILITY Back System Order Form

ROHO® understands that the needs of your clients are unique. For that reason, we are offering the Custom AGILITY back.

You can now use ROHO's DRY FLOATATION® technology to specifically address your client's postural needs. You determine exactly what air cells you need and where, the size of the air cells, and how many compartments of adjustable air are required.

### Order Form Example

#### STEP 1: Quick Release or Fixed Hardware Check one



##### Quick Release

Quick Release hardware makes removal for transport or storage a snap, even by those with limited hand dexterity. Simply unlock it and lift it by the handle.

##### Fixed

Fixed hardware is ideal for clients who rarely need to remove their replacement backs (available in heights 16 inches and lower).

Quick Release     Fixed


**STEP 2:** Each box on the featured shell can hold an air cell. Please determine where you would like air cells and the types of air cells needed.

- 1** 1" or 2.5 cm
- 2** LOW PROFILE® (2.25" x 5.5 cm)
- 3** MID PROFILE™ (3.25" x 8.5 cm)
- 4** HIGH PROFILE® (4.25" x 10.5 cm)

**STEP 3:** Custom AGILITY backs give you the options (or) option to create different adjustable air compartments. Please circle the compartments needed for this Custom AGILITY back.

**STEP 4:** Please note any special considerations, **especially valve locations**<sup>1</sup>, you would like our team to know about this custom AGILITY back.

#### SAMPLE:

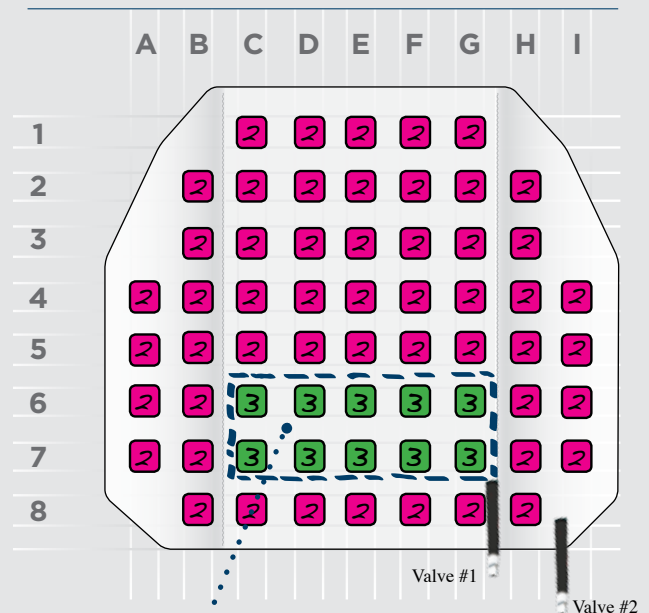

**STEP 3:** Needs an adjustable lumbar support. Use **3** air cells.

#### SAMPLE WHEELCHAIR BACK:

In this example, the clinician wanted MID PROFILE air cells in a separate adjustable lumbar support. The remaining cells are LOW PROFILE air cells that are also adjustable. Inflation valves come out of the bottom left of the AGILITY cover.



<sup>1</sup>Unless specified otherwise, valves will be placed toward the bottom of the custom AGILITY Back.

# ORDER FORM

Fits: AGILITY Minimum Contour 20" Width x 16" Height x 3" Depth

## STEP 1: Quick Release or Fixed Hardware

Check one.

	<p><b>Quick Release</b> Quick Release hardware makes removal for transport or storage a snap, even by those with limited hand dexterity. Simply unlock it and lift it by the handle.</p>
	<p><b>Fixed</b> Fixed hardware is ideal for clients who rarely need to remove their replacement backs (available in heights 16 inches and lower).</p>

Quick Release     Fixed

**STEP 2:** Each box on the featured shell can hold an air cell. Please determine where you would like air cells and the types of air cells needed.

- 1** 1" or 2.5 cm
- 2** LOW PROFILE® (2.25" x 5.5 cm)
- 3** MID PROFILE™ (3.25" x 8.5 cm)
- 4** HIGH PROFILE® (4.25" x 10.5 cm)

**STEP 3:** Custom AGILITY backs give you the options (or) option to create different adjustable air compartments. Please circle the compartments needed for this Custom AGILITY back.

**STEP 4:** Please note any special considerations, especially valve location<sup>1</sup>, you would like our team to know about this custom AGILITY back.

---



---



---




---

**PLEASE DO NOT SEND PATIENT-PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THIS PRODUCT.**

<sup>1</sup>Unless specified otherwise, valves will be placed toward the bottom of the custom AGILITY Back.

Please be advised that custom items take approximately 3 - 4 weeks from date of order to manufacture.

A B C D E F G H I J K

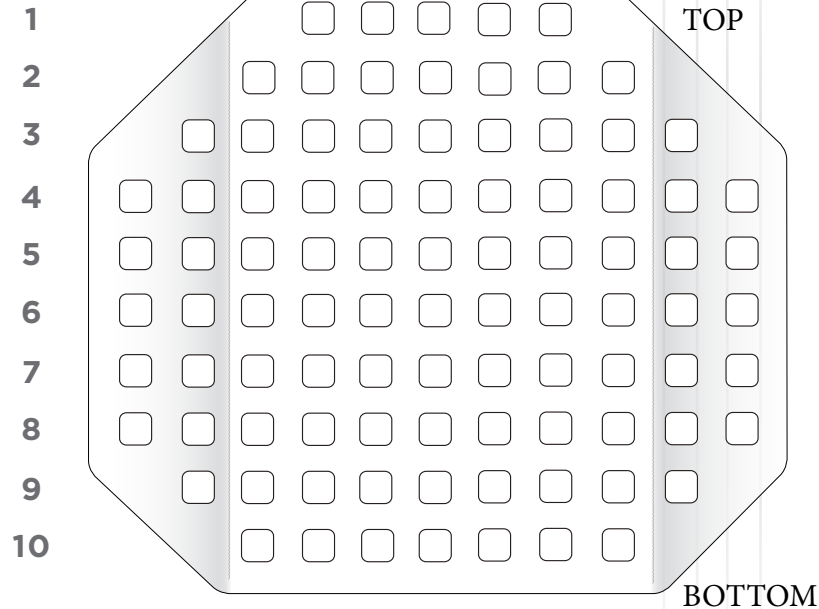

Provider/distributor name: \_\_\_\_\_

ROHO account #: \_\_\_\_\_

Circle one:                      **QUOTE**                      **ORDER**

Address line 1: \_\_\_\_\_

Address line 2: \_\_\_\_\_

City: \_\_\_\_\_

State: \_\_\_\_\_

ZIP: \_\_\_\_\_

Country: \_\_\_\_\_

Phone: \_\_\_\_\_ Fax: \_\_\_\_\_

E-mail: \_\_\_\_\_

Person ordering: \_\_\_\_\_

Reference name: \_\_\_\_\_

P.O.# (required to place an order): \_\_\_\_\_

Special instructions: \_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_



**100 North Florida Ave • Belleville, IL 62221-5429 • USA**

U.S.: 800 851 3449 • 618 277 9173 • fax 888 551 3449

Outside U.S.: 618 277 9150 fax 618 277 6518

Website: www.roho.com E-mail: cc@roho.com

©2014 ROHO, Inc. Manufactured by ROHO, Inc. The following are trademarks and registered trademarks of ROHO, Inc.: AGILITY™, DRY FLOATATION®, HIGH PROFILE®, LOW PROFILE®, MID PROFILE™, ROHO®. ROHO, Inc. has a policy of continual product improvement and reserves the right to amend this document.

\*Decisions about how to code a product are the responsibility of the provider/supplier. Since Medicare coding is subject to change, the provider should always confirm the HCPCS code and coverage criteria as part of the client assessment process.